

THE NEW DIABETES.SHOP EXPERIENCE QUICK START GUIDE

Supply ordering made easy.



Medtronic



PERSONALIZED HOME PAGE

- Upload a custom image and make the experience your own

TARGET SHIP DATE

- Helps you plan ahead, knowing in advance when your supplies are going to be shipped from Medtronic
- The new Diabetes.Shop displays your order's target ship date based on your last shipment date and product quantity, as well as insurance guidelines

ALL-IN-ONE ORDER STATUS

- See all you need to know about your supply order, 24/7 including:
 - Target ship date
 - Product and quantity details
 - Order progress
 - Any actions needed from you
- View additional orders, click or swipe through your order placards

CREATE ORDER

- Quickly set up scheduled orders or create a new one-time order

ORDER HISTORY

- View all your orders including orders that are in process, shipped, delivered, and canceled

MEDTRONIC ADVOCATE TEAM (VIRTUAL)


- Stay informed through personalized messages
- From start to finish, know how we are working with your doctor's office and insurance to complete your order – if we need more info, we'll ask – no need to call!

DEVICES

- Quickly see your current device on file

INSURANCE & BILLING

- View and update insurance
- See your pending balance and easily access the online payment portal




MANAGE SCHEDULED ORDERS

- Easily set-up, view, and personalize your automatic recurring shipments online, including target ship date, frequency, and quantity
- For those who are currently enrolled in the Auto Reorder program, also referred to as My Supply Connection (MSC), you can now easily view or manage automatic recurring shipments through the "Scheduled orders" page


ONE-TIME ORDER

- You also have the option to place a one-time order each time diabetes supplies are needed if you prefer not to have products set up on scheduled orders

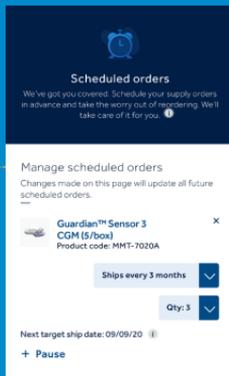

SCHEDULED ORDERS

- Products that are covered by insurance and/or require a prescription (i.e., sensors, reservoirs, infusion sets, etc.) can be placed on scheduled orders with the option to personalize the schedule; this is the best way to ensure uninterrupted flow of supplies
- You can also pause and resume scheduled order shipments based on your preferences

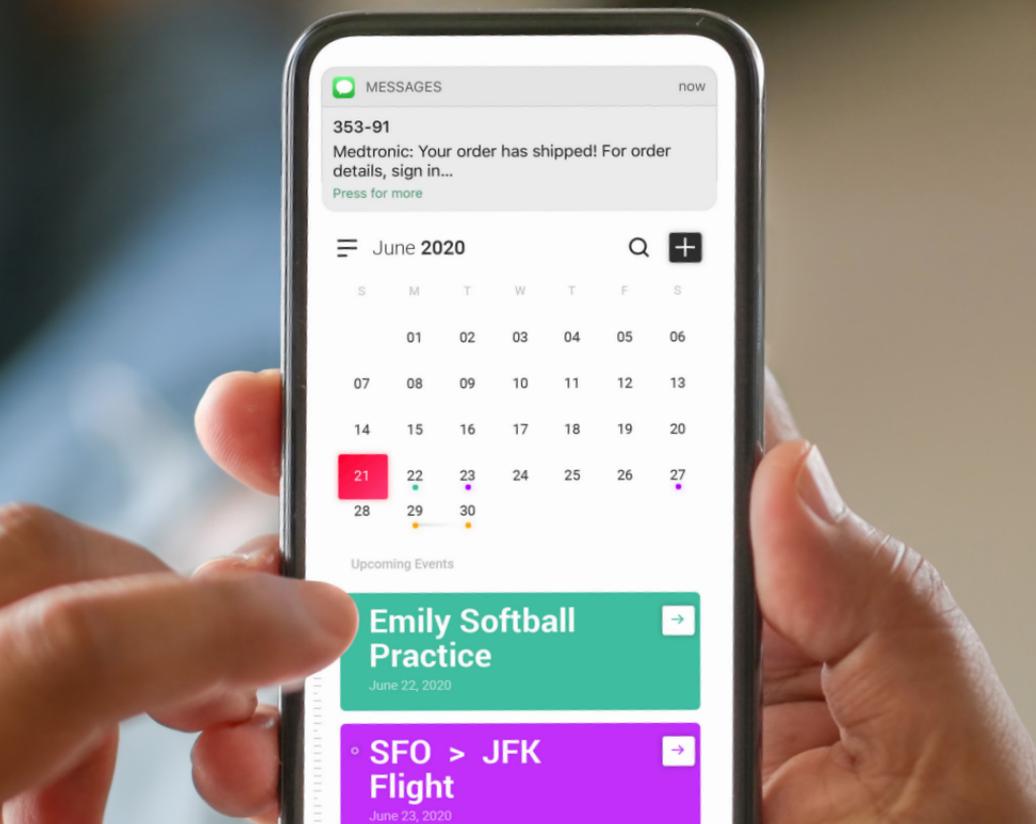

WHY CALL TO PLACE YOUR SUPPLY ORDER OR CHECK STATUS?

See all you need to know about
your supply order, 24/7.

Sign in today at www.Diabetes.Shop and
experience the **transformation.**

IMPORTANT SAFETY INFORMATION: MINIMED™ 670G SYSTEM

The Medtronic MiniMed™ 670G system is intended for continuous delivery of basal insulin (at user selectable rates) and administration of insulin boluses (in user selectable amounts) for the management of type 1 diabetes mellitus in persons, seven years of age and older, requiring insulin as well as for the continuous monitoring and trending of glucose levels in the fluid under the skin. The MiniMed™ 670G system includes SmartGuard™ technology, which can be programmed to automatically adjust delivery of basal insulin based on Continuous Glucose Monitor sensor glucose values and can suspend delivery of insulin when the sensor glucose value falls below or is predicted to fall below predefined threshold values. The system requires a prescription. The Guardian™ Sensor (3) glucose values are not intended to be used directly for making therapy adjustments, but rather to provide an indication of when a fingerstick may be required. A confirmatory finger stick test via the CONTOUR®NEXT LINK 2.4 blood glucose meter is required prior to making adjustments to diabetes therapy. All therapy adjustments should be based on measurements obtained using the CONTOUR® NEXT LINK 2.4 blood glucose meter and not on values provided by the Guardian™ Sensor (3). Always check the pump display to ensure the glucose result shown agrees with the glucose results shown on the CONTOUR® NEXT LINK 2.4 blood glucose meter. Do not calibrate your CGM device or calculate a bolus using a blood glucose meter result taken from an Alternative Site (palm) or from a control solution test. It is not recommended to calibrate your CGM device when sensor or blood glucose values are changing rapidly, e.g., following a meal or physical exercise. If a control solution test is out of range, please note that the result may be transmitted to your pump when in the “Always” send mode.

WARNING: Medtronic performed an evaluation of the MiniMed™ 670G system and determined that it may not be safe for use in children under the age of 7 because of the way that the system is designed and the daily insulin requirements. Therefore this device should not be used in anyone under the age of 7 years old. This device should also not be used in patients who require less than a total daily insulin dose of 8 units per day because the device requires a minimum of 8 units per day to operate safely.

Pump therapy is not recommended for people whose vision or hearing does not allow recognition of pump signals and alarms. Pump therapy is not recommended for people who are unwilling or unable to maintain contact with their healthcare professional. The safety of the MiniMed™ 670G system has not been studied in pregnant women. For complete details of the system, including product and important safety information such as indications, contraindications, warnings and precautions associated with system and its components, please consult <http://www.medtronicdiabetes.com/important-safety-information#minimed-670g> and the appropriate user guide at <http://www.medtronicdiabetes.com/download-library>.

940M21452-012 28FEB2020 © 2020 Medtronic. All rights reserved. Medtronic, Medtronic logo and Further, Together are trademarks of Medtronic.